



The penetration of the whole blood specimen in an embodiment of the present invention is as follows.

- The state after 30 seconds when the whole blood is added in one of embodiment in the present invention

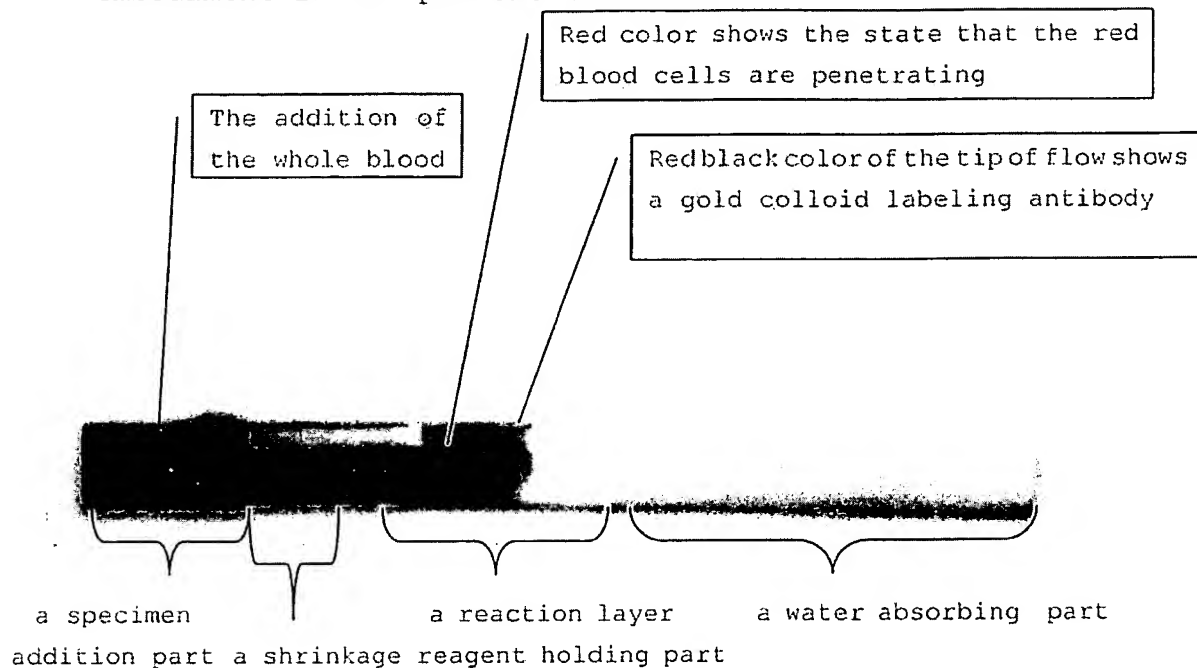

- ② The state after 45 seconds when the whole blood is added in an embodiment of the present invention

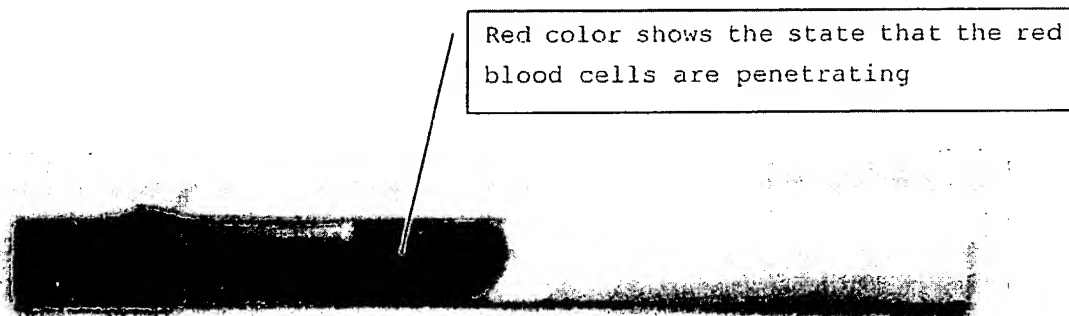

- ③ The state after 1 minute when the whole blood is added in an embodiment of the present invention

